

# DENGUE IgG QUANTI CARD

## Fluorescence immunoassay for qualitative detection of Dengue IgG antibodies in Human Serum/ Plasma

### INTRODUCTION

Dengue virus is a flavivirus found largely in areas of the tropic and sub-tropics. There are four distinct but antigenically related serotypes of dengue viruses, and transmission is by mosquito, principally *Aedes aegypti* and *Aedes albopictus*.

The mosquito-borne dengue viruses (serotype 1-4) cause dengue fever, a severe flu-like illness. The disease is prevalent in third world tropical regions and spreading to sub-tropical developed countries - including the United States. WHO estimates that 50-80 million cases of dengue fever occur worldwide each year, including a potentially deadly form of the disease called dengue hemorrhagic fever (DHF) and dengue shock syndrome (DSS). Primary infection with dengue virus results in a self-limiting disease characterized by mild to high fever lasting 3 to 7 days, severe headache with pain behind the eyes, muscle and joint pain, rash and vomiting. Secondary infection is the more common form of the disease in many parts of Southeast Asia and South America. IgM antibodies are not detectable until 5-10 days in case of primary dengue infection and until 4-5 days in secondary infection after the onset of illness. IgG appear after 14 days and persist for life in case of primary infection and rise within 1-2 days after the onset of symptoms in secondary infection. This form of the disease is more serious and can result in DHF and DSS. The major clinical symptoms can include high fever, hemorrhagic events, and circulatory failure, and the fatality rate can be as high as 40%. Early diagnosis of DSS is particularly important, as patients may die within 12 to 24 hours if appropriate treatment is not administered.

### INTENDED USE

Dengue IgG Quanti Card is a sensitive immuno- chromatographic test for the qualitative detection of dengue IgG antibodies in human Serum/ Plasma with iQuant Analyzer. This test is for in vitro diagnostic use only and is intended as an aid in the diagnosis of dengue infection.

### PRINCIPLE

Dengue IgG Quanti Card is a fluorescence immunoassay. The test area is coated with dengue antigen (1-4). When a sample is added to the device, dengue IgG antibodies in the sample react with anti-human IgG antibodies complex to fluorescent dye in the conjugate. On addition of Assay Buffer, this complex migrates along the nitrocellulose membrane to the test region and forms an antibody-antigen-antibody fluorescence immunocomplex. The result will be displayed by iQuant Analyzer.

### MATERIALS PROVIDED

Dengue IgG Quanti Card kit contains following components to perform the assay:

- Dengue IgG Quanti Card Device
- Assay Buffer
- Instruction Manual

### KIT PRESENTATION














24 Test Pack                      48 Test Pack                      96 Test Pack

### STORAGE AND STABILITY


The kit should be stored at 2-8°C in the coolest and driest area available. Expiry date on the kit indicates the date beyond which kit and its components should not be used. Dengue IgG Quanti Card should not be frozen and must be protected from exposure to humidity.

### DESCRIPTION OF SYMBOLS USED

The following are graphical symbols used in or found on J. Mitra diagnostic products and packing. These symbols are the most common ones appearing on medical devices and their packing. They are explained in more detail in the British and European Standard EN ISO 15223-1:2016.

 Manufactured By	 In vitro diagnostic medical device
 No. of tests	 See Instruction for use
 Lot Number Batch Number	 Temperature Limitation
 Manufacturing Date	 Caution, see instruction for use
 Expiry Date	 Catalogue Number
 Do not use if package is damaged	 Keep away from sunlight
 Single use only	

### WARNING FOR USERS

 CAUTION: ALL THE SAMPLES TO BE TESTED SHOULD BE HANDLED AS THOUGH CAPABLE OF TRANSMITTING INFECTION. NO TEST METHOD CAN OFFER COMPLETE ASSURANCE THAT HUMAN BLOOD PRODUCTS WILL NOT TRANSMIT INFECTION.

- The use of disposable gloves and proper biohazardous clothing is STRONGLY RECOMMENDED while running the test.

- In case there is a cut or wound in hand, DO NOT PERFORM THE TEST.
- Do not smoke, drink or eat in areas where specimens or kit reagents are being handled.
- Tests are for in vitro diagnostic use only and should be run by competent person only.
- Do not pipette by mouth.
- All materials used in the assay and samples should be decontaminated in 5% sodium hypochlorite solution for 30-60 min. before disposal or by autoclaving at 121°C at 15psi for 60 min. Do not autoclave materials or solution containing sodium hypochlorite. They should be disposed off in accordance with established safety procedures.
- Wash hands thoroughly with soap or any suitable detergent, after the use of the kit. Consult a physician immediately in case of accident or contact with eyes, in the event that contaminated material are ingested or come in contact with skin puncture or wounds.
- Spills should be decontaminated promptly with Sodium Hypochlorite or any other suitable disinfectant.
- Assay Buffer contains Sodium Azide as a preservative. If these material are to be disposed off through a sink or other common plumbing systems, flush with generous amounts of water to prevent accumulation of potentially explosive compounds. In addition, consult the manual guideline "Safety Management No. CDC-22", Decontamination of Laboratory Sink Drains to remove Azide salts" (Centre for Disease Control, Atlanta, Georgia, April 30, 1976).
- Follow standard biosafety guidelines for handling & disposal of potentially infective material.

### PRECAUTIONS

In order to obtain reproducible results, the following instructions must be followed:

- Do not use the kit beyond the expiry date.
- Do not mix reagents from different batches.
- Do not open the foil pouch until it attains room temperature.
- Do not re-use the test cartridge.
- Follow the given test procedure and storage instructions strictly.
- Do not temper / paste any sticker or write anything on the QR-Code as this will lead to erroneous result.
- Do not touch the membrane with the pipette tip.


**Important Note: Dengue IgG Quanti Card is only operational in conjunction with iQuant Analyzer.**

### SAMPLE / SPECIMEN COLLECTION AND STORAGE

- Serum/ Plasma samples may be used with this test.
- For plasma, collect the whole blood in a clean container (containing EDTA, sodium fluoride or heparin) by venipuncture. Fresh samples are preferred for testing as they perform best when tested immediately after collection. If specimens cannot be tested immediately, they should be refrigerated at 2-8°C. For storage for more than 3 days, freeze the specimen at -20°C or below.
- Repeated freezing and thawing of the specimen should be avoided.
- Specimens containing precipitate or particulate matter may yield inconsistent test results. Such specimens must be centrifuged and the clear supernatant should only be used for testing.
- The use of hemolytic, lipaemic, icteric or bacterially contaminated specimens should be avoided as it may lead to erratic results.


### BEFORE YOU START

The Assay Buffer Solution provided in the kit has closed nozzle and screw cap with pin (outside). Before using Assay Buffer, keep the vial vertically straight and tap down gently on the working platform, so that Assay Buffer comes down at the bottom of the vial. To orifice/puncture the closed nozzle, follow the instruction as illustrated below:

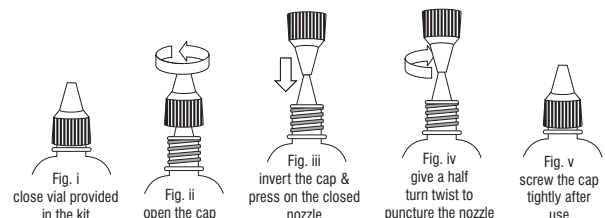

## TEST PROCEDURE

1. Bring the complete kit and specimen to be tested to room temperature prior to testing. RT  
20-30°C
2. Remove the test cartridge from the foil pouch prior to use and place it on a flat and dry surface. The test should be performed immediately after removing the test card from the foil pouch.
3. Label the test cartridge with patient's name or identification number. **Do not write on QR code.**
4. Add 10µl Serum/ Plasma sample using micropipette onto the sample pad in the sample well 'S'. **Care should be taken to avoid any spillage on the QR Code.**

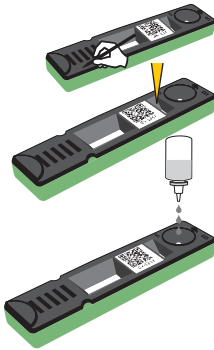

NOTE : Make sure that the sample from the micropipette has been completely transferred to the sample pad.

5. Add 3 drops of the Assay Buffer in the buffer well 'B'.
6. Allow the reaction to occur for 40 minutes.
7. Insert the test cartridge into the i-Quant Analyzer with arrow (←) marked side on the top of cartridge facing towards the analyzer and press RUN icon. Note down the value displayed on the screen of i-Quant Analyzer & interpret the result as mentioned below.
8. Discard the Dengue IgG Quanti Card immediately after reading results at 40 minutes considering it to be potentially infectious.

**Important Note: Do not read results after 40 minutes.**

## INTERPRETATION OF RESULTS

The iQuant Analyzer will display results as Reactive, Equivocal or Non-Reactive as follows:

**IgG Reactive: > 1.1 U and above:** interpret the result as Dengue IgG Antibody reactive.

**Equivocal: > 0.9 to ≤ 1.1 U:** Interpret the result as equivocal. Repeat the test after centrifuging the sample at 5000 rpm for 20 minutes. Even after repeating the test, if result comes equivocal, further test the sample with alternative method or collect another sample.

**Non-Reactive: Below ≤ 0.9 U:** Interpret the result as Dengue IgG Antibody non-reactive.

## LIMITATIONS AND INTERFERENCES

1. The test is for in vitro diagnostic use only.
2. This test detects the presence of Dengue IgG antibodies to dengue virus in the specimen and should not be used as the sole criteria for the diagnosis of Dengue virus infection.
3. Serological cross-reactivity across the Flavivirus group (St. Louis encephalitis, Japanese encephalitis, West Nile and yellow fever virus) is common.
4. As with all diagnostic tests, all results must be correlated with other clinical findings. If the test result is negative and clinical symptoms persist, additional follow-up testing using other clinical methods is recommended. A negative result at any time does not preclude the possibility of an early infection of Dengue virus.
5. This is only a screening test. Therefore, isolation of virus, antigen detection in fixed tissues, RT-PCR and serological test like haemagglutination inhibition test, more specific alternative diagnosis method must be used in order to obtain a confirmation of dengue virus infection.

## PERFORMANCE CHARACTERISTICS OF DENGUE IgG QUANTI CARD

The kit has been evaluated in-house with the known panel of fresh as well as frozen Dengue IgG antibody positive and Negative samples. The performance of the test kit was evaluated and compared with the a license commercially available ELISA test kit. The samples included cross-reacting samples; Epstein-Barr virus, Malaria, Rheumatoid factor, Leptospirosis, Japanese encephalitis, yellow fever and West Nile viruses. Following is the in-house evaluation.

Sample Type	No. of Samples tested	Result of Dengue IgG ELISA test		Dengue IgG Quanti Card	
		Positive	Negative	Positive	Negative
Negative	855	0	855	12	843
Dengue IgM Positive	120	0	120	0	120
Dengue IgG Positive	75	75	0	74	1

Sensitivity: **97.23%**

Specificity: **97.36%**

## Precision:

### Intra assay precision

Within run (Intra assay) precision have been determined by testing 10 replicates of two negative and five dengue IgG antibody positive samples (weak, medium & strong). The C.V. (%) of all the samples were within 10% of the unit.

## Inter assay precision (Reproducibility)

Between run (Inter assay) precision have been determined by testing 10 replicates of two negative and five Dengue IgG antibody positive samples (3 weak, 1 medium & 1 strong) in 10 sequential days. The C.V. (%) of all the samples were within 10% of the unit.

## LIMITED EXPRESSED WARRANTY DISCLAIMER

The manufacturer limits the warranty to the test kit, as much as that the test kit will function as an in vitro diagnostic assay within the limitations and specifications as described in the product instruction-manual, when used strictly in accordance with the instructions contained therein. The manufacturer disclaims any warranty expressed or implied including such expressed or implied warranty with respect to merchantability, fitness for use or implied utility for any purpose. The manufacturer's liability is limited to either replacement of the product or refund of the purchase price of the product and in no case liable to claim of any kind for an amount greater than the purchase price of the goods in respect of which damages are likely to be claimed. The manufacturer shall not be liable to the purchaser or third parties for any injury, damage or economic loss, howsoever caused by the product in the use or in the application there of.

## TROUBLE SHOOTING

PROBLEM	POSSIBLE CAUSE	SOLUTION
1. False negative	a) Low sample volume along with less volume of Assay Buffer used.	Repeat the test with proper volume of samples and/or Assay Buffer.
2. False positive	a) Less volume of Assay Buffer added/used.	Repeat the test with proper volume of Assay Buffer.

## BIBLIOGRAPHY OF SUGGESTED READING

1. Dengue: guidelines for diagnosis, treatment, prevention and control –New Edition WHO/HTM/NTD/DEN/2009.1
2. Rapid Dengue Diagnosis: A prospective study using a Commercial RapidTest\* (S.K. Lam+ and L.C.S. Lum++)
3. Dengue disease diagnosis: A puzzle to be solved Jaime Eduardo Castellanos 1.2. Carolina Coronel-Ruiz1 Rev. Fac. Med. 2014 Vol. 62 No. 4:617-629

For in-vitro diagnostic use only, not for medicinal use

## J. MITRA & CO. PVT. LTD.

A 180-181, Okhla Indl. Area, Phase-1, New Delhi-110 020, INDIA

Ph: +91-11-47130300, 47130500, 26818971-73

e-mail: jmitra@jmitra.co.in Internet: www.jmitra.co.in